



Title:


## Certificate of Analysis (CoA)

**Date:** 5/28/2026  
**Date Tested:** 5/25/2026  
**Customer:** CURO  
**Testing material:** Bac\_Water  
**Lot Number:** BAC03SR526  
**BT Sample ID:** 005000040193039  
**Labeled Peptide Content/Potency:** 3 mL  
**Storage:** R.T.  
**Visual Description:** Small clear vial: white sample, white label, silver crimp, dark blue plastic cap.  
**Labeled as:** Bac\_Water  
**Manufacturer:** Jinzhou Hongbai Technology Co., Ltd.  
**Testing Purpose:** FTIR and HPLC analysis for the identification, purity, potency and composition of a water product. It does not provide information on particulate matter, microbial contamination or presence of endotoxins.




Test	Method	Specification	Result
General Appearance	USP <630>	clear liquid	clear liquid
Mass	USP <41>	As recorded	3 mL
FTIR Identification and Composition Analysis	USP <197A>	Sample spectrum should confirm the content of water via characteristic bands	FTIR sample spectrum confirms the presence of Bac_Water.
HPLC Purity of Peptide Assay	USP <621>	Specifications: $\geq 98\%$	99.7%
HPLC Potency Assay	USP <621>	Specifications: 90 – 110%	0.8 mg (8.8%)

The results of the CoA relate only to the item(s) tested and applied to the sample as received.

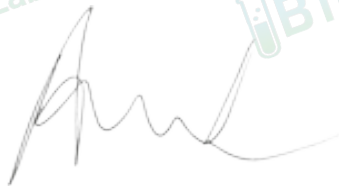

Andrea Castro, AS  
Scientist-II  
BTLabs

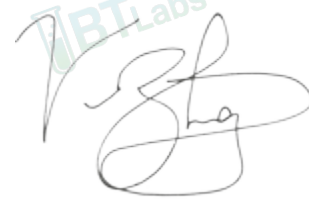


Verna Zheng, AS  
Scientist-II  
BTLabs




Title:

## Certificate of Analysis (CoA)

### FTIR ID and Composition Analysis: Bac Water Lot BAC03SR526

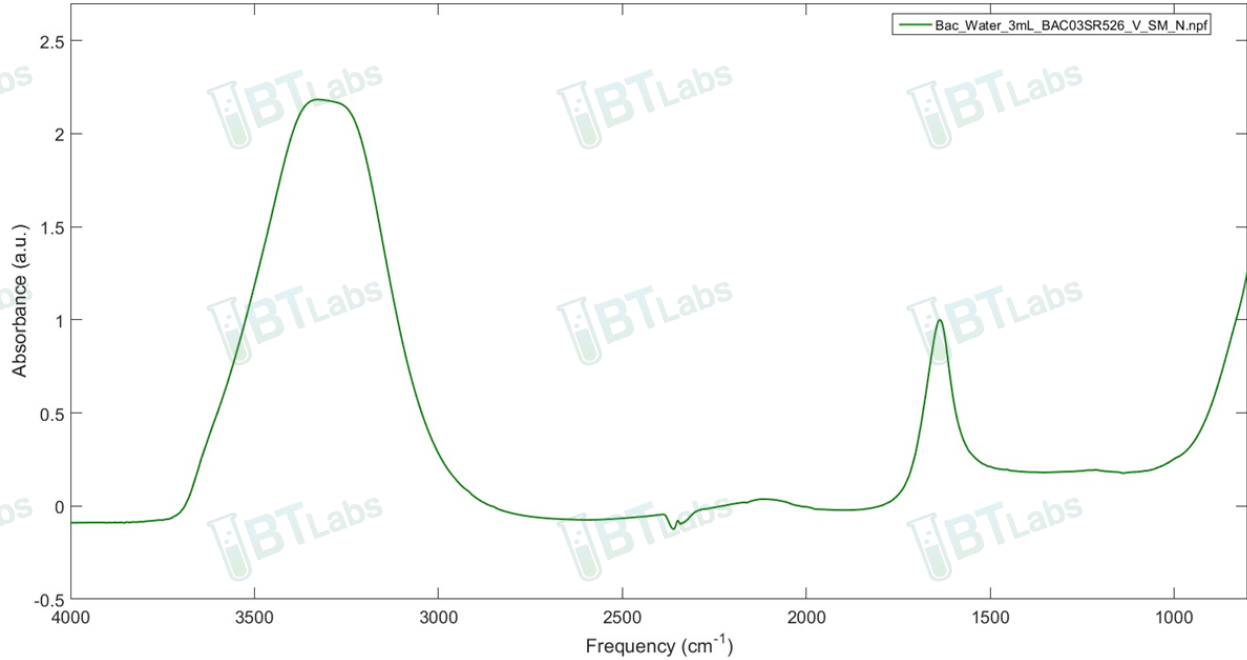

### HPLC Purity and Potency Assay @ 220 nm: Bac Water Lot BAC03SR526

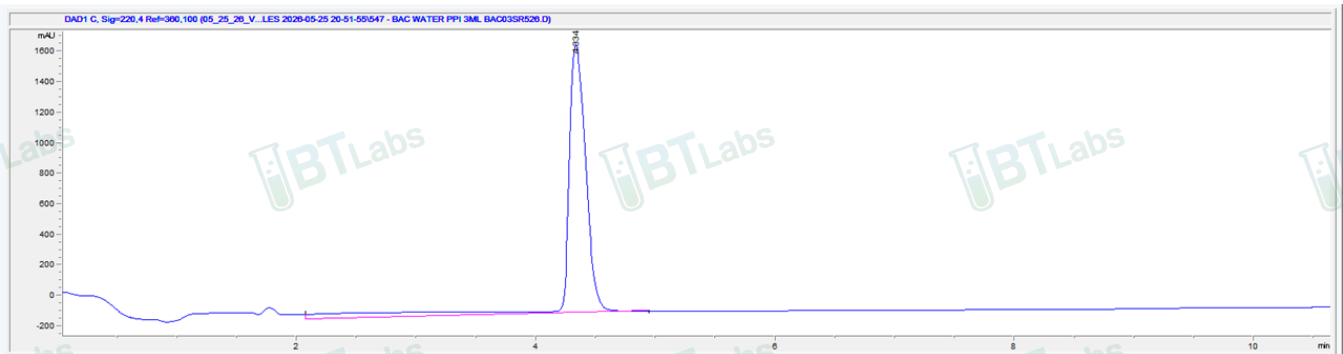

#### **Bac Water Lot BAC03SR526 @ 220 nm**

Peak #:	Retention Time (min)	Area (mAU*s)
1	4.334	19574.1



Title:

## Certificate of Analysis (CoA)

### pH Test BAC Water Lot BAC03SR526

Sample ID	Description	Volume (mL)	pH Run1	pH Run2	pH Run3
BAC03SR526	BAC Water	1	6.13	6.10	6.11